

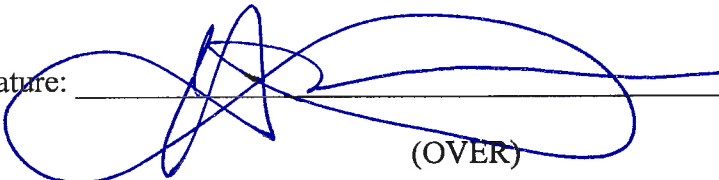
# VERIFICATION OF CALIBRATION REPORT

OCT 29 2010

Of DataMaster cdm Breath test Instrument

State of Alaska

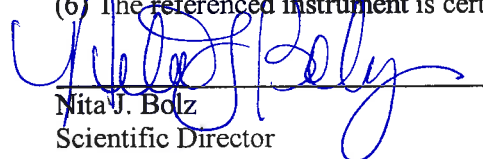
Scientific Crime Detection Laboratory – Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N: <u>130193</u> ✓
Name: <u>JAMES C. GIPSON</u>		ID#: <u>4842</u> ✓ Date: <u>28 Oct 10</u> ✓
<b>A</b>	Agency: <u>Palmer Police Department</u> Phone #: <u>(907) 745-4811</u>	
Instrument Location: <u>Palmer Police Department</u>		
Alco S/N: <u>718493</u> ✓ Target Value: <u>.084</u> ✓ High Pressure: <u>400</u>		
<b>B</b>	Alco Test Value Average: <u>.083</u> ✓ 1 <sup>st</sup> Alco 2 <sup>nd</sup> Alco	
Signature: 		(OVER)


(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 22<sup>nd</sup> day of DEC, 2010.

  
Daniel L. Nicholas  
Notary Public, State of Alaska  
Commission Expires with Office

(Notary Seal Stamp)



# VERIFICATION OF CALIBRATION REPORT

*Of DataMaster cdm Breath test Instrument*

*State of Alaska*

*Scientific Crime Detection Laboratory – Statewide Breath Alcohol Program*

DataMaster cdm S/N: 130193

(CONTINUED FROM FRONT PAGE)

**C**

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130193

OCTOBER 28, 2010

OPERATOR'S NAME:

GIPSON/JAMES/C

OPERATOR'S NUMBER: 4842

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

RJCS9

O.L. #: 0123456

DEPT/AGENCY: PLM1

CASE/REPORT: 01-2345

TEST TYPE: U

ALCO TARGET VALUE: .004

ALCO S/N: 718493

--- BREATH ANALYSIS ---

.004 ADJUSTED FOR 29.23 in  
ALCO TARGET .002 12:53  
BLANK TEST .000 12:54  
INTERNAL STANDARD VERIFIED 12:54  
ALCO TV 29.23 in .003 12:54  
BLANK TEST .000 12:55  
SUBJECT SAMPLE .000 12:56  
BLANK TEST .000 12:56  
ALCO TV 29.23 in .003 12:57  
BLANK TEST .000 12:57

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130193

OCTOBER 28, 2010

TIME 12:50

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 01/08/09  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 41c  
BAROMETER: 29.23 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

!@#%&'()\*+,-./:0123456789:;<=>?@ABCDEF6  
HIJKLMNPOQRSTUVWXYZ[\]^\_`abcedefghijklmno  
pqrsstuvwxyz{|}~